

NI PXIe-5630 Specifications

RF Vector Network Analyzer

This document lists specifications for the NI PXIe-5630 RF vector network analyzer (NI 5630).

Specifications are warranted under the following conditions:

- Minimum of 30 minutes warm-up time
- No averaging applied to the data
- Environmental ambient temperature of $23\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$
- Less than $1\text{ }^{\circ}\text{C}$ ambient temperature deviation after user calibration
- Calibration cycle maintained
- Type-K, $50\ \Omega$ connectors used
- Chassis fan speed set to High
- Onboard Reference clock applied
- NI-VNA version 1.0 or later used

Specifications describe the warranted, traceable product performance over ambient temperature ranges of $23\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$, unless otherwise noted.

Typical values describe useful product performance beyond specifications that are not covered by warranty and do not include guardbands for measurement uncertainty or drift. Typical values may not be verified on all units shipped from the factory. Unless otherwise noted, typical values cover the expected performance of units over ambient temperature ranges of $23\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$ with a 90% confidence level, based on measurements taken during development or production.

Nominal values (or supplemental information) describe additional information about the product that may be useful, including expected performance that is not covered under *Specifications* or *Typical* values. Nominal values are not covered by warranty.

Specifications are subject to change without notice. For the most recent NI 5630 specifications, visit ni.com/manuals.

To access NI 5630 documentation, navigate to **Start»All Programs»National Instruments»NI-VNA»Documentation**.



Hot Surface If the NI 5630 has been in use, component modules or their shields may exceed safe handling temperatures and may cause burns. Allow the NI 5630 to cool before touching shields on component modules or removing modules from the chassis.

Electromagnetic Compatibility Guidelines

This product was tested and complies with the regulatory requirements and limits for electromagnetic compatibility (EMC) as stated in the product specifications. These requirements and limits are designed to provide reasonable protection against harmful interference when the product is operated in its intended operational electromagnetic environment.

This product is intended for use in industrial locations. There is no guarantee that harmful interference will not occur in a particular installation, when the product is connected to a test object, or if the product is used in residential areas. To minimize the potential for the product to cause interference to radio and television reception or to experience unacceptable performance degradation, install and use this product in strict accordance with the instructions in the product documentation.

Furthermore, any changes or modifications to the product not expressly approved by National Instruments could void your authority to operate it under your local regulatory rules.



Caution To ensure the specified EMC performance, operate this product only with shielded cables and accessories.

Contents

General Information	3
Port 1 Source Characteristics	4
Port 2 Receiver Characteristics	5
Measurement Speed	6
Corrected System Performance	6
Corrected System Performance with K-Type Connectors with NI Manual Calibration Kit and Precision Cables	6
Corrected System Performance with N-Type Connectors with NI Manual Calibration Kit and Precision Cables	10
Corrected System Performance with K-Type Connectors and NI AutoCal Kit and Precision Cables	14
Trigger	18
Reference Frequency	19
Calibration	19
Power	19
Hardware Front Panels and Connectors	20
Dimensions and Weight	22

Environmental.....	22
Operating Environment.....	22
Storage Environment	22
Shock and Vibration	23
Safety	23
Electromagnetic Compatibility	23
CE Compliance	24
Online Product Certification.....	24
Environmental Management.....	24

General Information

Measurand.....	S11, S21
IF bandwidth (IFBW).....	10 Hz, 30 Hz, 100 Hz, 300 Hz, 1 kHz, 3 kHz, 10 kHz, and 30 kHz
Sweep capability	
Maximum frequency.....	6 GHz
Minimum frequency	10 MHz
Resolution	10 Hz
Minimum number of points	1
Maximum number of points	3,201
Frequency spacing	Linear, shown in the following equation: $\frac{\text{Stop Freq} - \text{Start Freq}}{\# \text{ of Points}}$
NI-VNA soft front panel (SFP)	
sweep modes.....	Single sweep and hold, continuous, and continuous wave (CW)
Data formats	Magnitude (log), magnitude (linear), phase, group delay, VSWR, impedance, reflection/transmission coefficient, real, imaginary
NI-VNA SFP display types.....	Value vs. frequency plot, Smith chart
Number of averages	4,096 maximum

Smoothing.....25% maximum

User calibration

 MethodsAutoCal, manual

 Types1-port SOL, 1-path 2-port SOLT, transmission response, and reflection response

Port 1 Source Characteristics

Frequency range10 MHz to 6 GHz

Frequency resolution10 Hz

Frequency accuracy2.5 ppm + Internal or External Timebase Aging + Internal or External Timebase Temperature Stability

Internal timebase

 Aging±1 ppm

 Temperature stability±2.5 ppm/°C

Power range+5 dBm to -30 dBm

Power accuracy

 At +5 dBm test port power±2 dB

 At any test port power±4 dB, typical

Power step resolution.....0.5 dB

Harmonics (measured at +5 dBm source power)

Frequency	Harmonic	Typical
10 MHz to <250 MHz	<-6 dBc	<-8 dBc
250 MHz to <1.7 GHz	<-9 dBc	<-12 dBc
1.7 GHz to <2.5 GHz	<-16 dBc	<-20 dBc
2.5 GHz to 6.0 GHz	<-22 dBc	<-28 dBc

Nonharmonic spurs

(at +5 dBm source power)<-14 dBc, <-17 dBc, typical

Port 2 Receiver Characteristics

0.1 dB compression point..... >+5 dBm, typical

Noise floor¹

Frequency	Range	Typical
10 MHz to <3 GHz	<-113 dBm/Hz	<-115 dBm/Hz
3 GHz to 6 GHz	<-105 dBm/Hz	<-110 dBm/Hz

Raw input match 18 dB

Dynamic range²

Frequency	Range	Typical
10 MHz to <3 GHz	>108 dB	>110 dB
3 GHz to 6 GHz	>100 dB	>105 dB

Trace noise (measured at +5 dBm with 100 Hz IF bandwidth)

Frequency	Noise	Typical
10 MHz to <3.0 GHz	<6 mdB rms	<3 mdB rms
3.0 GHz to 6.0 GHz	<9 mdB rms	<5 mdB rms

Damage input level 23 dBm

¹ Calculated from maximum port power and dynamic range.

² Measured at +5 dBm with 10 Hz IF bandwidth in high-sensitivity mode and an RF calibration with isolation using the NI manual calibration kit into 50 Ω terminations.

Measurement Speed¹

Span	IFBW	Number of Points		
		201	801	3201
Zero Span (Continuous Wave Mode)	30 kHz	28 ms	93 ms	350 ms
	1 kHz	230 ms	874 ms	3,452 ms
Small Span: 1 GHz to 2 GHz	30 kHz	79 ms	262 ms	958 ms
	1 kHz	273 ms	1,036 ms	4,054 ms
Full Span: 10 MHz to 6 GHz	30 kHz	79 ms	283 ms	1,057 ms
	1 kHz	272 ms	1,057 ms	4,161 ms

All values typical. Time Domain operations add 0.5 ms per 100 points.

Corrected System Performance

Corrected System Performance with K-Type Connectors with NI Manual Calibration Kit and Precision Cables

Specification	Frequency	
	10 MHz to <5 GHz	5 GHz to 6 GHz
Directivity	42 dB	36 dB
Source Match	35 dB	35 dB
Load Match	18 dB	18 dB

¹ Indicates the amount of time it takes after hardware configuration has been committed to the device to initiate a sweep, perform the measurement, and then fetch the data from the device. Measurements taken using an NI PXIe-8133 controller and an NI PXIe-1065 chassis. Benchmarks run on a single device at a time.

Transmission Uncertainty

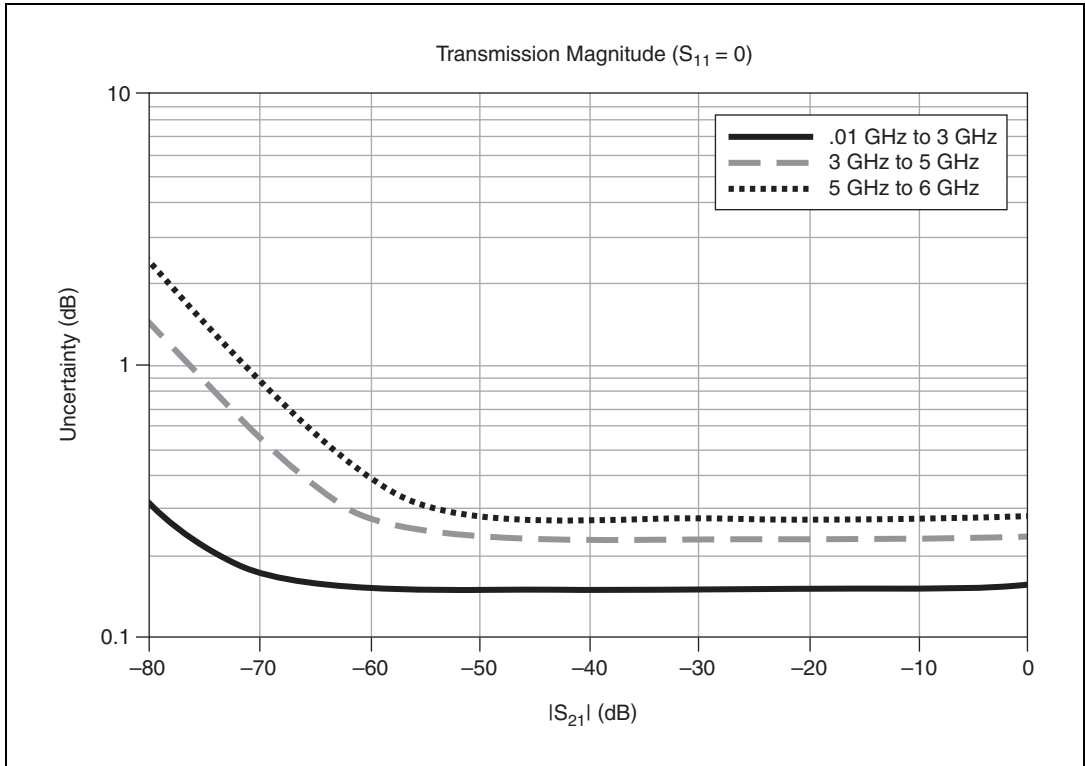


Figure 1. Magnitude Uncertainty

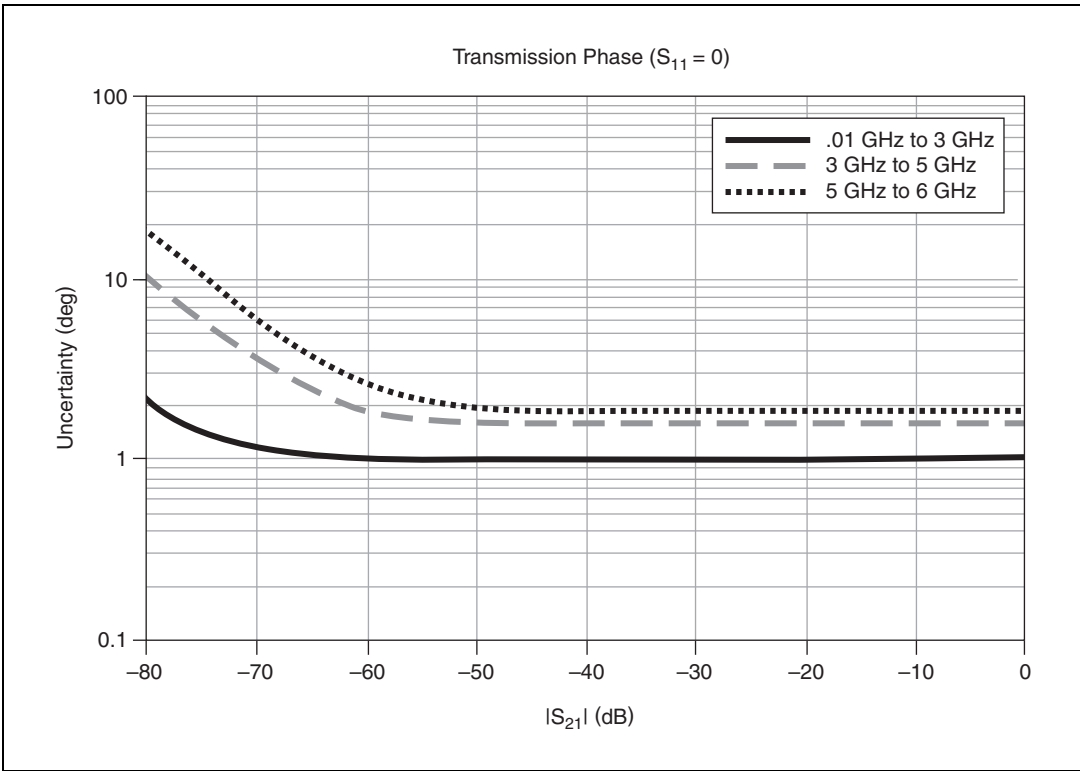


Figure 2. Phase Uncertainty

Reflection Uncertainty

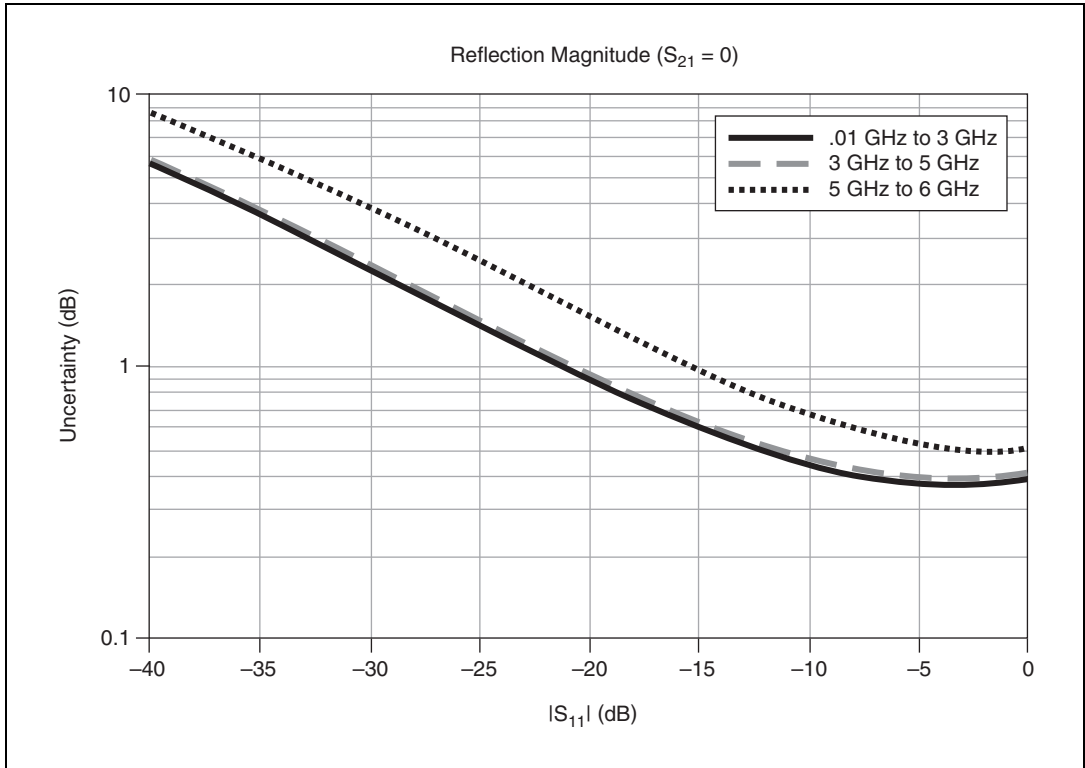


Figure 3. Magnitude Uncertainty

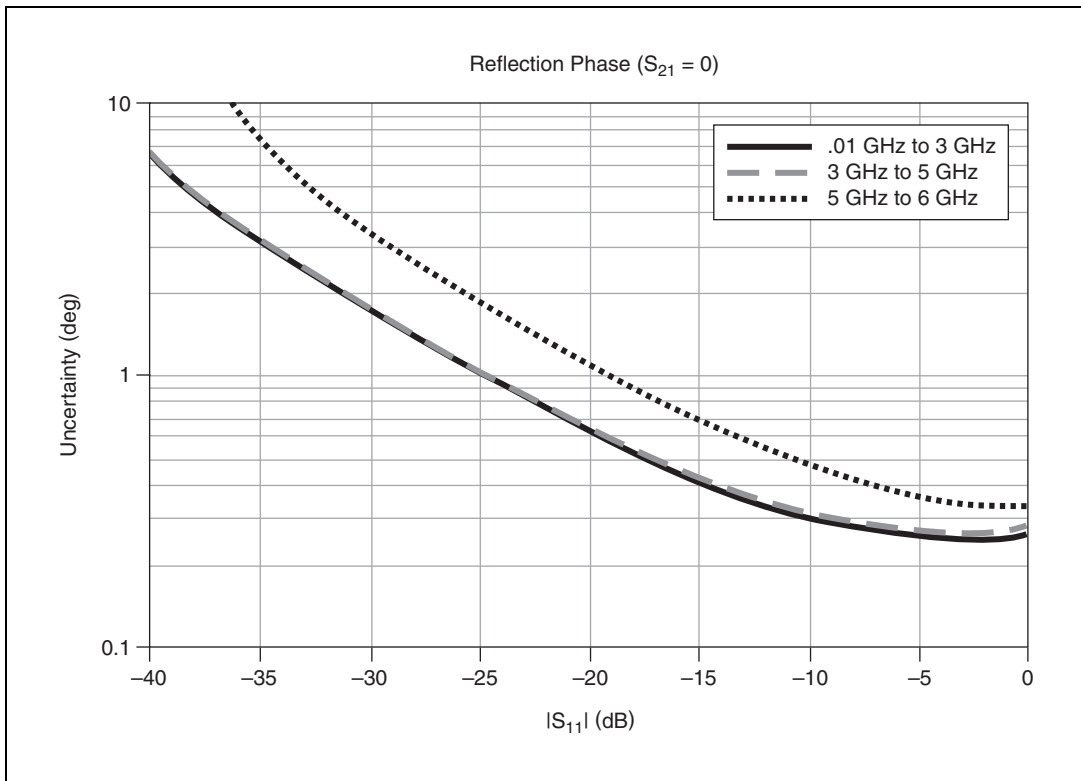


Figure 4. Phase Uncertainty

Corrected System Performance with N-Type Connectors with NI Manual Calibration Kit and Precision Cables

Specification	Frequency	
	10 MHz to <5 GHz	5 GHz to 6 GHz
Directivity	42 dB	36 dB
Source Match	35 dB	35 dB
Load Match	18 dB	18 dB

Transmission Uncertainty

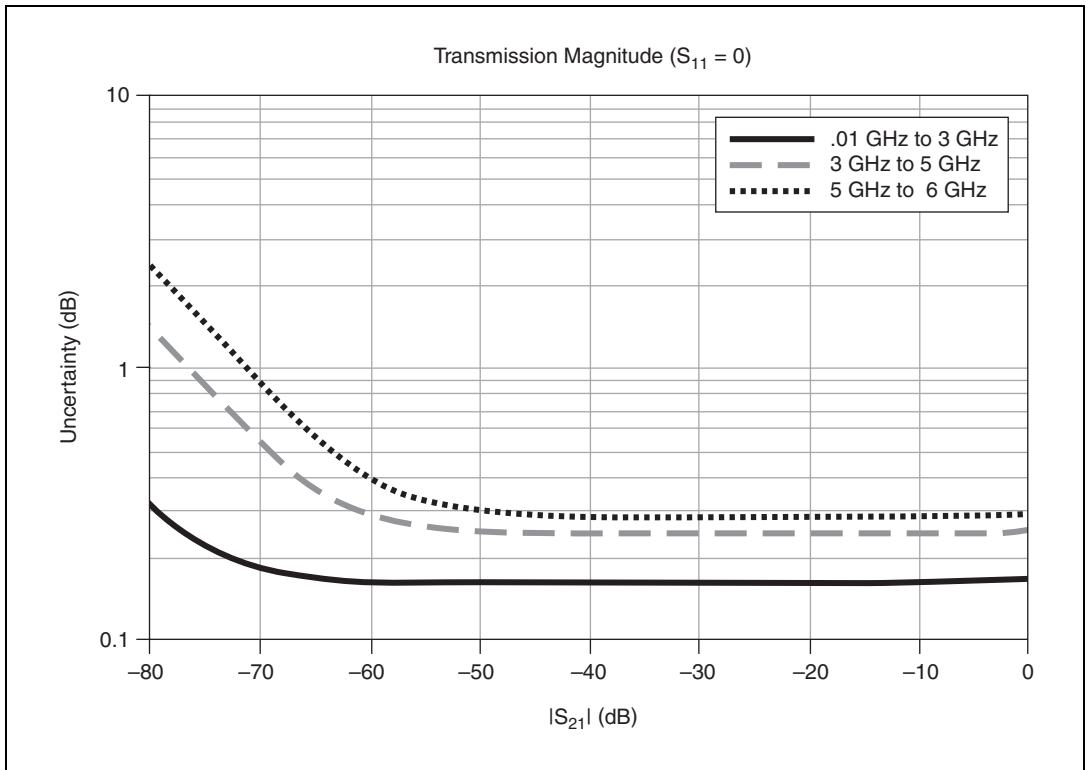


Figure 5. Magnitude Uncertainty

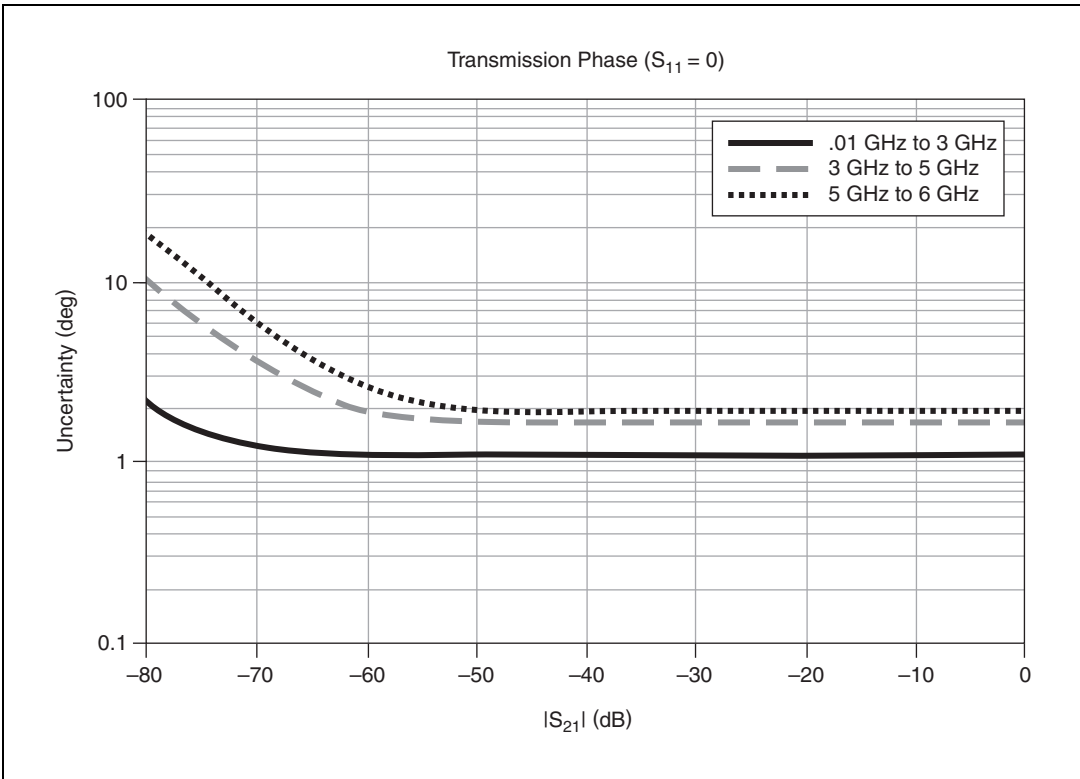


Figure 6. Phase Uncertainty

Reflection Uncertainty

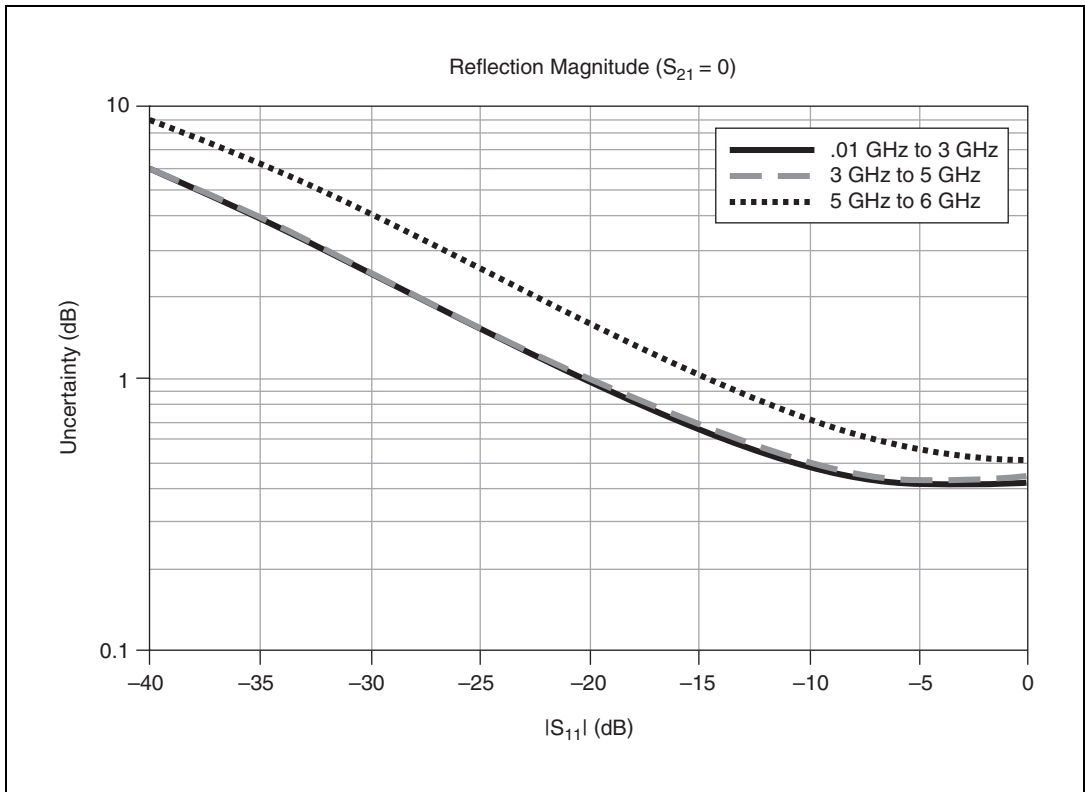


Figure 7. Magnitude Uncertainty

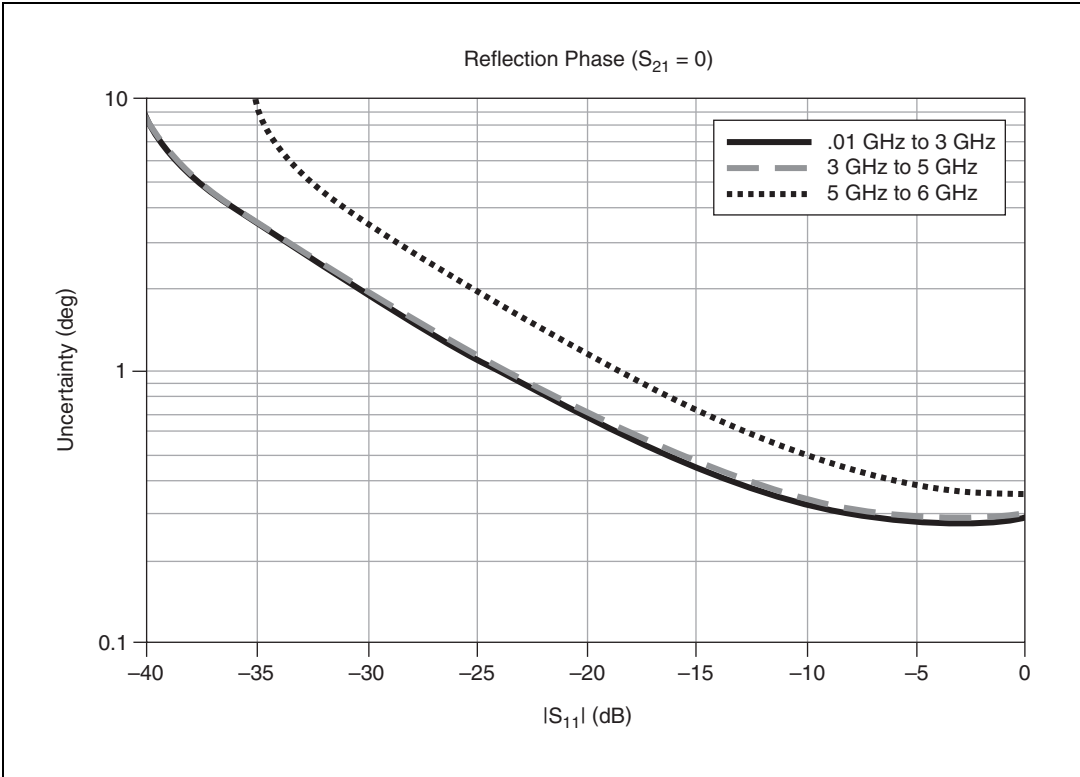


Figure 8. Phase Uncertainty

Corrected System Performance with K-Type Connectors and NI AutoCal Kit and Precision Cables

Specification	Frequency	
	10 MHz to <5 GHz	5 GHz to 6 GHz
Directivity	42 dB	36 dB
Source Match	35 dB	35 dB
Load Match	18 dB	18 dB

Transmission Uncertainty

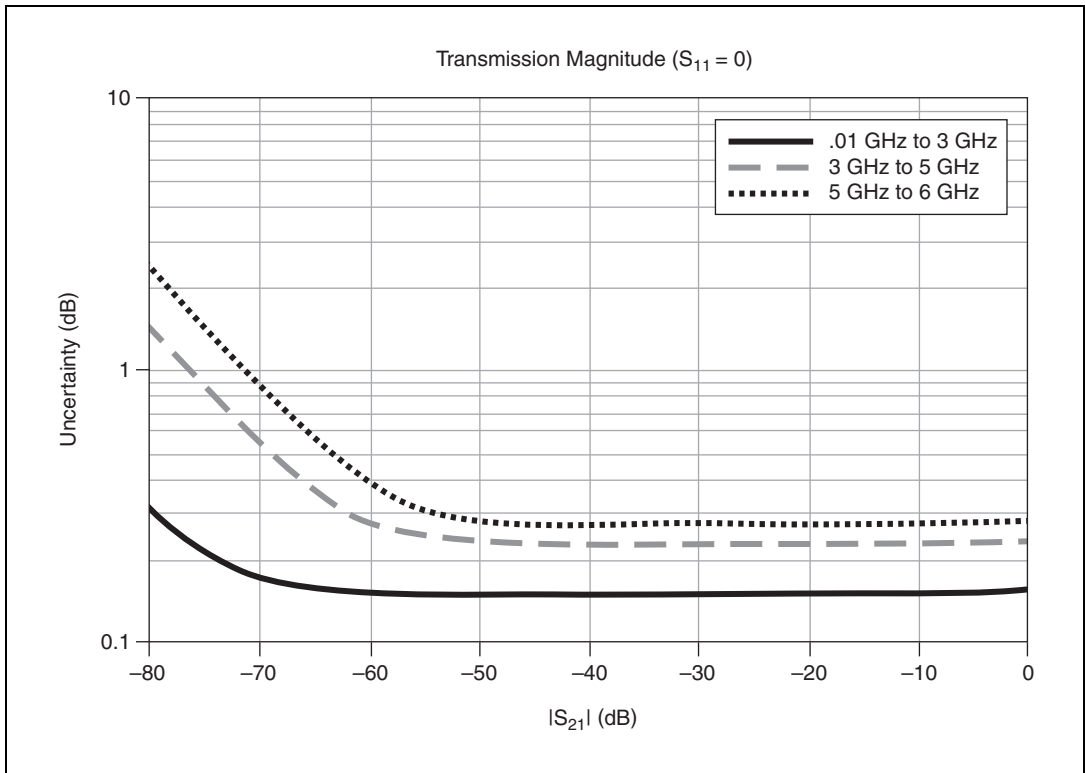


Figure 9. Magnitude Uncertainty

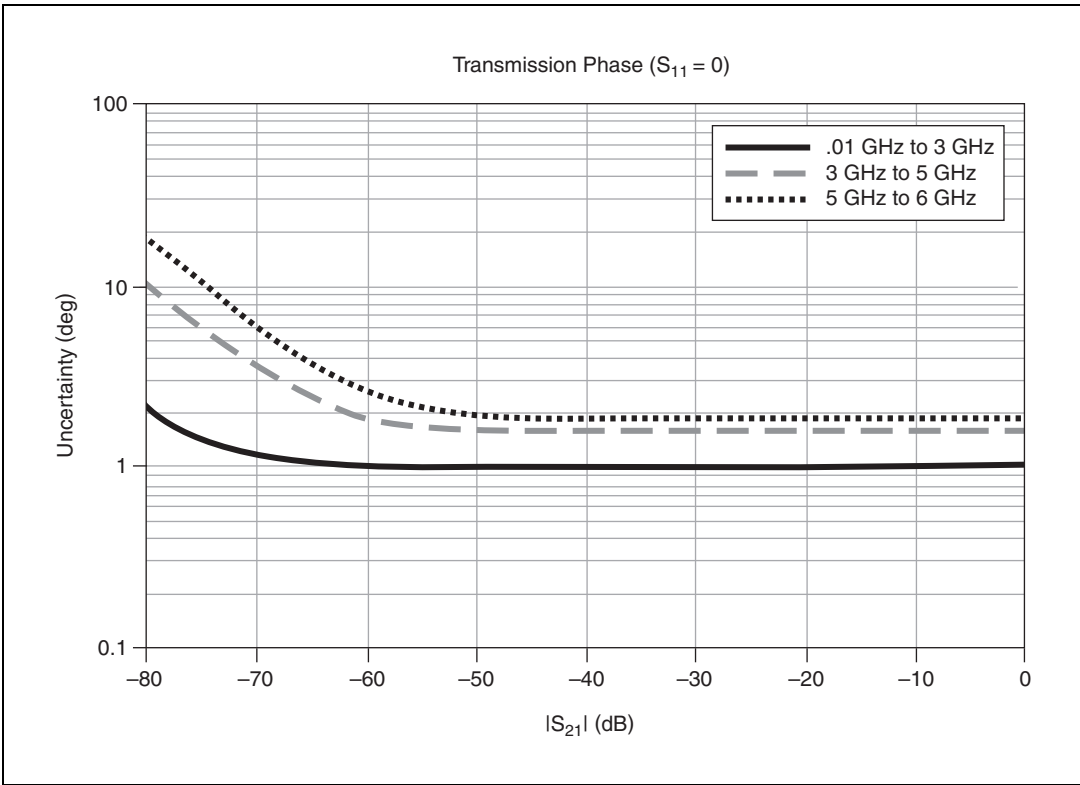


Figure 10. Phase Uncertainty

Reflection Uncertainty

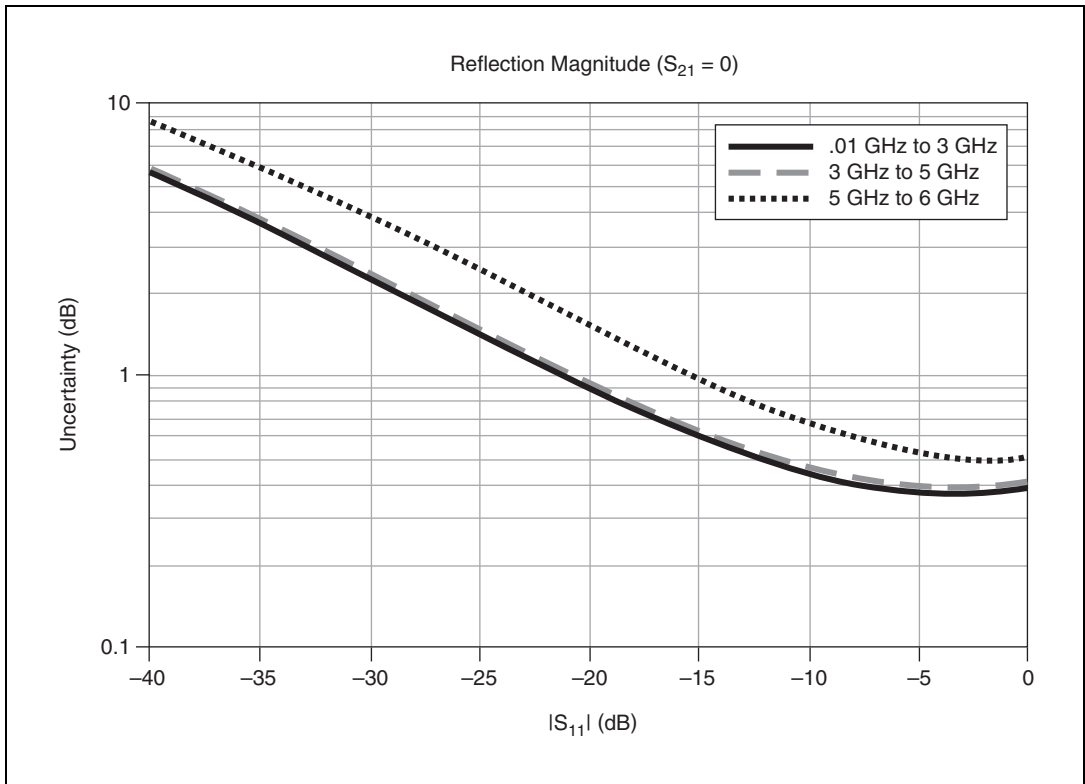


Figure 11. Magnitude Uncertainty

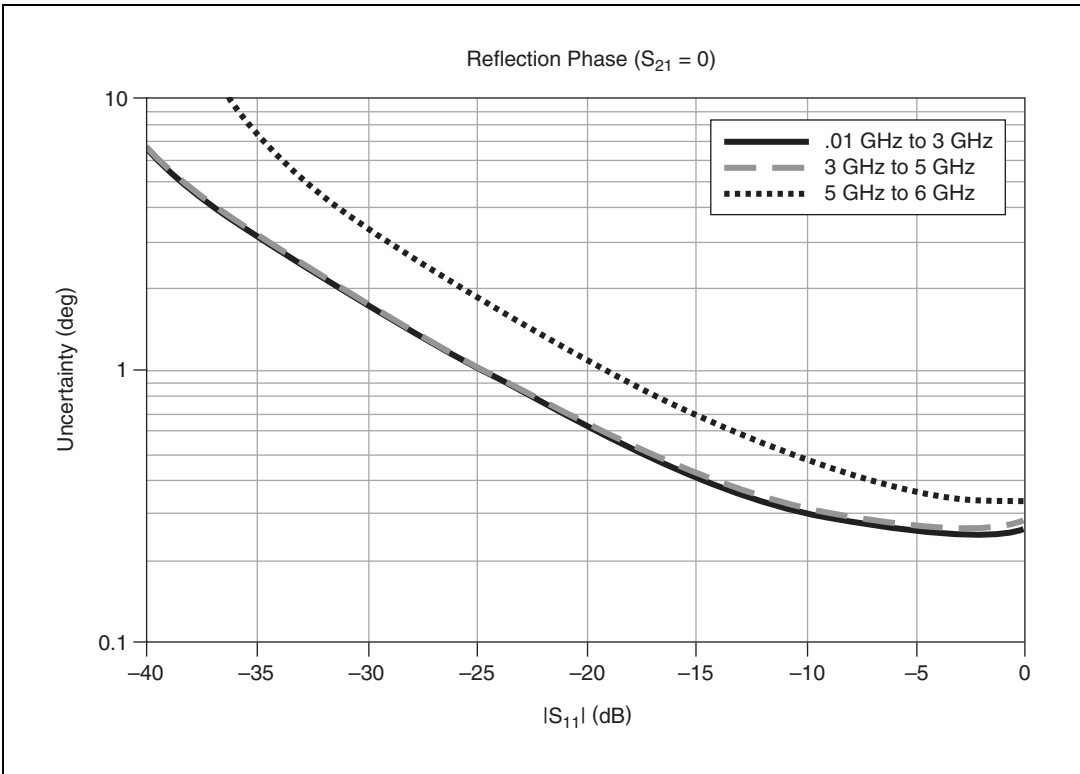


Figure 12. Phase Uncertainty

Trigger

Start trigger types.....Immediate, software, digital edge

Digital edge Start trigger sourcesPFI 0, PXI_Trig<0..7>

Input range+3.3 V logic (+5 V tolerant)

Minimum trigger width

PFI 050 ns

PXI_Trig<0..7>50 ns

Reference Frequency

Frequency sources.....	Onboard, REF IN
Input impedance.....	50 Ω
Input range.....	+3 dBm to -10 dBm sine wave
Frequency range.....	10 MHz \pm 10 ppm

Calibration

Interval.....	1 year (from first device use after external calibration)
---------------	---

Power

3.3 VDC.....	640 mA, typical
12 VDC.....	950 mA, typical

Hardware Front Panels and Connectors

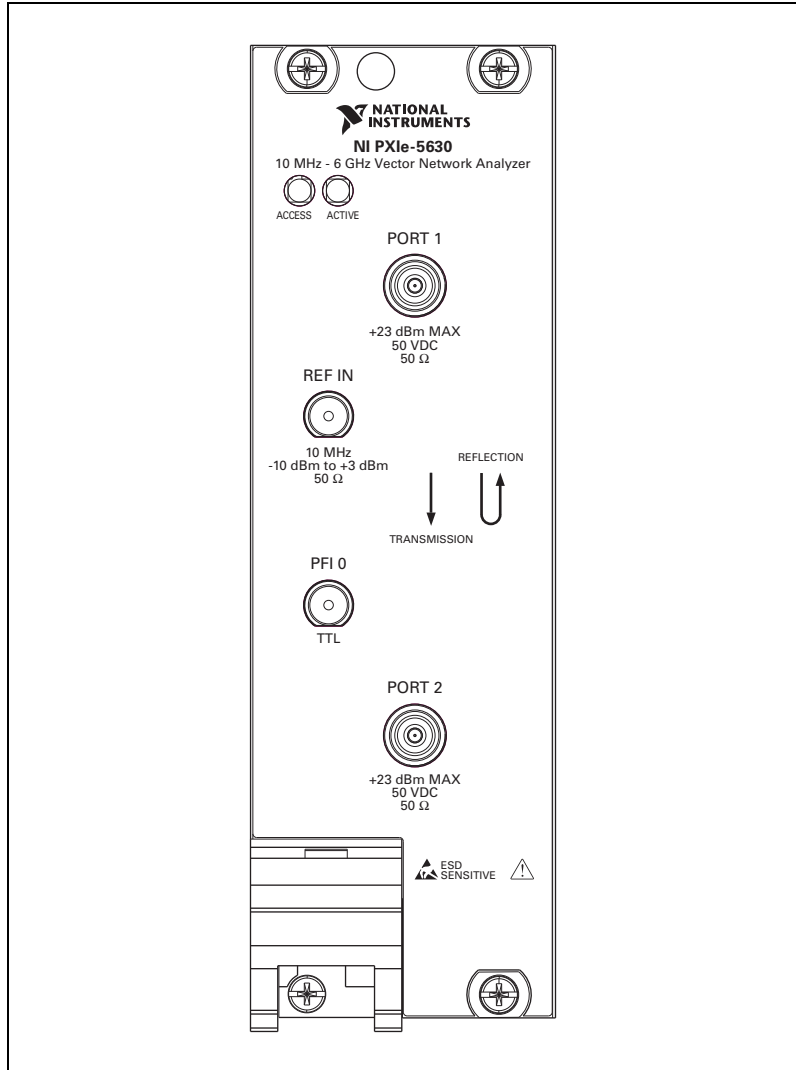


Figure 13. NI 5630 Front Panels

The following table provides more information about the connectors located on the NI 5630 front panel.

Table 1. NI 5630 Front Panel Connectors

Connector	Type	Function
PORT 1	Type-K	Input/output terminal for NI 5630 measurements. Refer to the Port 1 Source Characteristics section for more information about this connector.
REF IN	SMA	Input terminal for an external reference signal for the NI 5630. Refer to the Reference Frequency section for more information about this connector.
PFI 0	SMA	Input terminal for an external trigger signal. This connector is 3.3 V TTL logic (+5 V tolerant). Refer to the Trigger section for more information about this connector.
PORT 2	Type-K	Input terminal for NI 5630 measurements. Refer to the Port 2 Receiver Characteristics section for more information about this connector.

The following table provides LED and indication information for the LEDs located on the NI 5630 front panel.

Table 2. NI 5630 Front Panel LEDs

LED	Indication
ACCESS	<p>Indicates the basic hardware status of the NI 5630 module.</p> <p>OFF—The module is not yet functional.</p> <p>AMBER—The module is being accessed. Accessed means that the device is being communicated with over the PXI Express bus.</p> <p>GREEN—The module is ready to be programmed by NI-VNA.</p> <p>RED—The module has detected a hardware error, such as a hardware failure. The LED remains red until the error condition is removed.</p>
ACTIVE	<p>Indicates the state of the NI 5630 module.</p> <p>OFF—The module is not yet functional.</p> <p>AMBER—The module is armed and waiting for a trigger.</p> <p>GREEN—The module has received a Start trigger. This state also indicates that the module is making a measurement.</p> <p>RED—The module has detected a spurious error, such as when the PLL becomes unlocked. The LED remains red until the error condition is removed.</p>

Dimensions and Weight

Dimensions	3U, two slot, PXI Express module, 21.6 cm × 4.0 cm × 13.0 cm (8.5 in. × 1.6 in. × 5.1 in.)
Weight	680 g (24.0 oz)

Environmental

Specifications in this document are guaranteed under the following specified environmental conditions unless otherwise stated.

Altitude0 m to 2,000 m

Pollution Degree2

Indoor use only.

Operating Environment

Warm-up time30 minutes

Ambient temperature range0 °C to 55 °C
(Tested in accordance with
IEC 60068-2-1 and
IEC 60068-2-2. Meets
MIL PRF-28800F Class 3
low temperature limit and
MIL PRF-28800F Class 2
high temperature limit.)

Relative humidity range.....10% to 90%, noncondensing
(Tested in accordance with
IEC 60068-2-56.)

Storage Environment

Ambient temperature range-41 °C to +71 °C
(Tested in accordance with
IEC 60068-2-1 and
IEC 60068-2-2. Meets
MIL PRF-28800F Class 3 limits.)

Relative humidity range.....5% to 95%, noncondensing
(Tested in accordance with
IEC 60068-2-56.)

Shock and Vibration

Operating Shock..... 30 g peak, half-sine, 11 ms pulse
(Tested in accordance
with IEC 60068-2-27. Meets
MIL PRF-28800F Class 2 limits.)

Random Vibration

Operating 5 Hz to 500 Hz, 0.3 g_{rms}

Non-operating 5 Hz to 500 Hz, 2.4 g_{rms}
(Tested in accordance with
IEC 60068-2-64. Nonoperating
test profile exceeds the
requirements of
MIL PRF-28800F, Class 3.)

Safety

This product is designed to meet the requirements of the following standards of safety for electrical equipment for measurement, control, and laboratory use:

- IEC 61010-1, EN 61010-1
- UL 61010-1, CSA 61010-1



Note For UL and other safety certifications, refer to the product label or the [Online Product Certification](#) section.

Electromagnetic Compatibility

This product meets the requirements of the following EMC standards for electrical equipment for measurement, control, and laboratory use:

- EN 61326-1 (IEC 61326-1): Class A emissions; Basic immunity 1
- EN 55011 (CISPR 11): Group 1, Class A emissions
- AS/NZS CISPR 11: Group 1, Class A emissions
- FCC 47 CFR Part 15B: Class A emissions
- ICES-001: Class A emissions



Note In the United States (per FCC 47 CFR), Class A equipment is intended for use in commercial, light-industrial, and heavy-industrial locations. In Europe, Canada, Australia and New Zealand (per CISPR 11) Class A equipment is intended for use only in heavy-industrial locations.



Note Group 1 equipment (per CISPR 11) is any industrial, scientific, or medical equipment that does not intentionally generates radio frequency energy for the treatment of material or inspection/analysis purposes.



Note For EMC declarations and certifications, refer to the *Online Product Certification* section.

CE Compliance

This product meets the essential requirements of applicable European Directives, as amended for CE marking, as follows:

- 2006/95/EC; Low-Voltage Directive (safety)
- 2004/108/EC; Electromagnetic Compatibility Directive (EMC)

Online Product Certification

To obtain product certifications and the Declaration of Conformity (DoC) for this product, visit ni.com/certification, search by model number or product line, and click the appropriate link in the Certification column.

Environmental Management

NI is committed to designing and manufacturing products in an environmentally responsible manner. NI recognizes that eliminating certain hazardous substances from our products is beneficial to the environment and to NI customers.

For additional environmental information, refer to the *NI and the Environment* Web page at ni.com/environment. This page contains the environmental regulations and directives with which NI complies, as well as other environmental information not included in this document.

Waste Electrical and Electronic Equipment (WEEE)



EU Customers At the end of the product life cycle, all products *must* be sent to a WEEE recycling center. For more information about WEEE recycling centers, National Instruments WEEE initiatives, and compliance with WEEE Directive 2002/96/EC on Waste and Electronic Equipment, visit ni.com/environment/weee.

电子信息产品污染控制管理办法（中国 RoHS）



中国客户 National Instruments 符合中国电子信息产品中限制使用某些有害物质指令 (RoHS)。关于 National Instruments 中国 RoHS 合规性信息，请登录 ni.com/environment/rohs_china。(For information about China RoHS compliance, go to ni.com/environment/rohs_china.)

LabVIEW, National Instruments, NI, ni.com, the National Instruments corporate logo, and the Eagle logo are trademarks of National Instruments Corporation. Refer to the *Trademark Information* at ni.com/trademarks for other National Instruments trademarks. Other product and company names mentioned herein are trademarks or trade names of their respective companies. For patents covering National Instruments products/technology, refer to the appropriate location: **Help>Patents** in your software, the `patents.txt` file on your media, or the *National Instruments Patents Notice* at ni.com/patents. Refer to the *Export Compliance Information* at ni.com/legal/export-compliance for the National Instruments global trade compliance policy and how to obtain relevant HTS codes, ECCNs, and other import/export data.